


Titel reagent red cells release

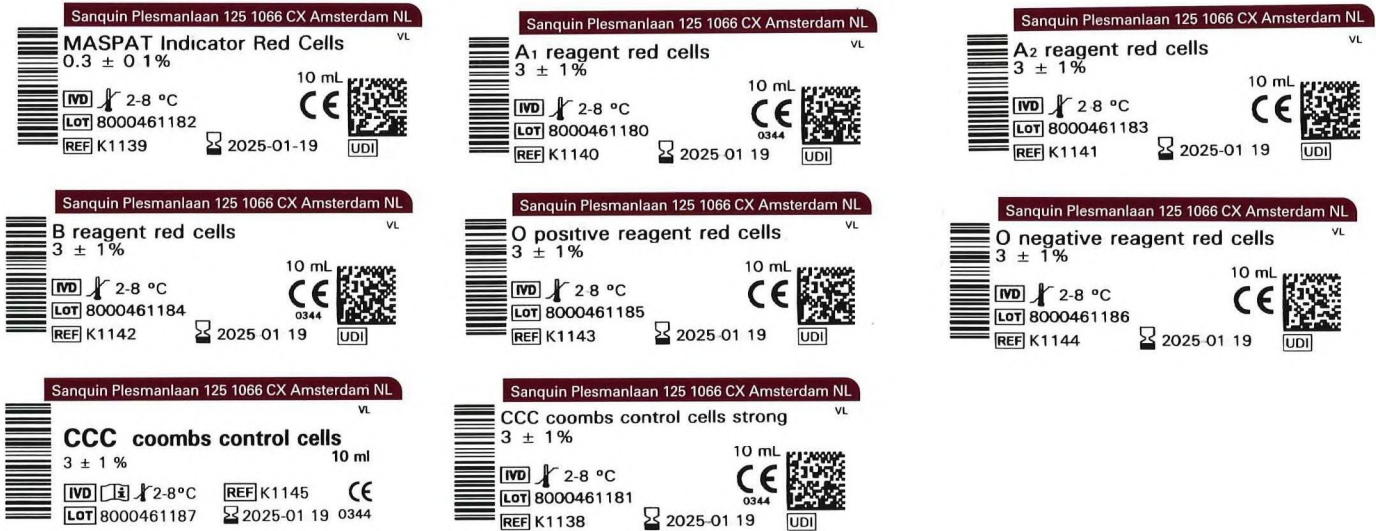

Analysis	Requirement								Result
		anti-A	anti-B	anti-A ₁	anti-D	DAT	IAT control		
Antigen control	MIRC	0.3%	0	0	n.t.*	n.t.*	≥ 2+	n.t.*	Conform requirements
	A ₁	3%	≥ 3+	0	≥ 3+	n.t.*	0	n.t.*	Conform requirements
	A ₂	3%	≥ 2+	0	0	n.t.*	0	n.t.*	Conform requirements
	B	3%	0	≥ 3+	n.t.*	n.t.*	0	n.t.*	Conform requirements
	O ^{positive}	3%	0	0	n.t.*	≥ 2+	0	n.t.*	Conform requirements
	O ^{negative}	3%	0	0	n.t.*	0	0	n.t.*	Conform requirements
	CCC	3%	0	0	n.t.*	n.t.*	≥ 2+	1+ ≥ ≤ 2+	Conform requirements
	CCCstrong	3%	0	0	n.t.*	n.t.*	≥ 3+	1+ ≥ ≤ 3+	Conform requirements
Hematocrit	MIRC	0.3 ± 0.1%							Conform requirements
	All other cells	3 ± 1%							Conform requirements

All the donor units used in the production of this reagent have been tested for the markers of specific disease transmitting agents in accordance with current EU guidelines to GMP and found to be non reactive.

*n.t.: not tested.

Approved by

Date: 05 December 2024

QA/QC: 

VERTROUWELIJK